




Return electrodes

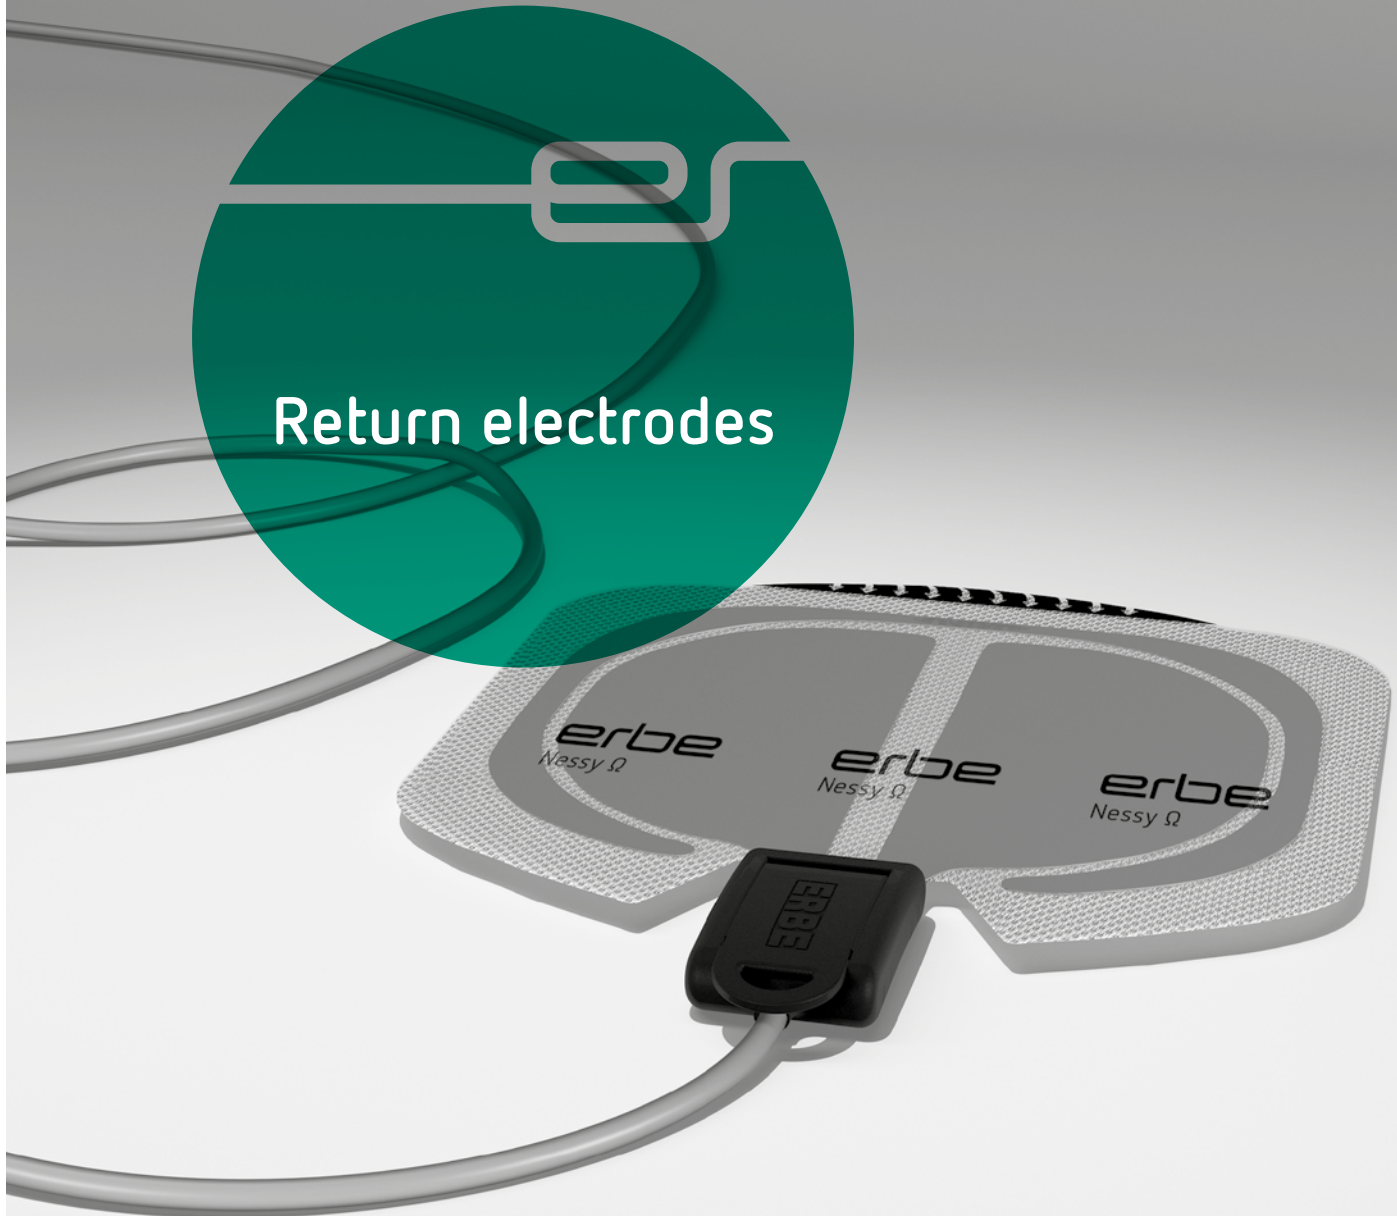

Legend


Important notes

The authors and Erbe Elektromedizin GmbH have taken the greatest possible care while compiling the catalogue with electrosurgical accessories. Nevertheless, it is impossible to exclude the possibility that errors may be contained herein.

The information and recommendations given here may not be construed as constituting any basis for any claims against Erbe Elektromedizin GmbH. Should legal regulations stipulate liability, such liability shall be limited to intentional misconduct or gross negligence.

The data on the use of instruments is based on clinical experience. Medical science is subject to a process of permanent change based on research and clinical experience. Therefore the products are subject to alterations in design and technique. Because of production tolerances dimensions in the catalogue may marginally differ.

Further product information

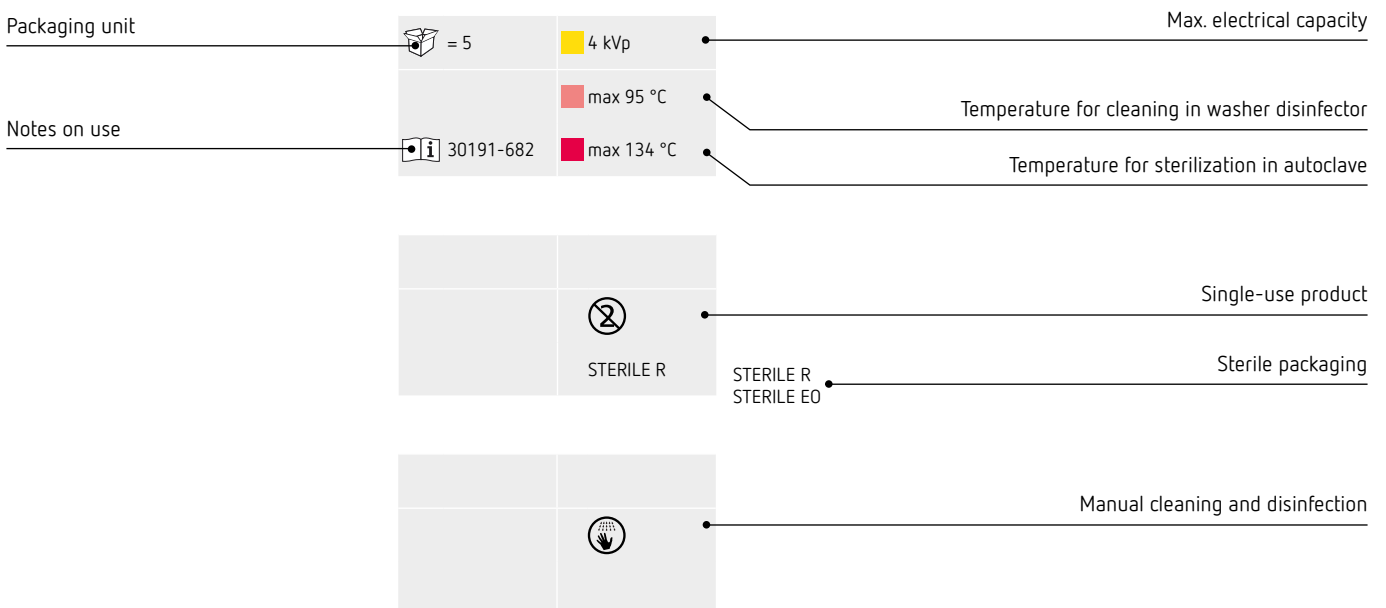

Please read carefully the corresponding notes on use before using any instrument.

Electrosurgery

Return electrodes

- 04 Single-use with contact stud
- 05 Single-use with connecting cable
- 06 Reusable with contact stud

Return electrodes

Single-use with contact stud

Erbe Nessy Ω , split, VIO, contact surface 85 cm²



equipotential ring 23 cm², without connecting cable


No. 20193-082

= 50

30193-082



Erbe NESSY Plate 170, split, VIO, ICC, ACC, contact surface 168 cm²



without connecting cable


No. 20193-070

= 50

30193-080



Erbe NESSY Plate 70, split, VIO, ICC, ACC, contact surface 72 cm²



without connecting cable, for children from 5 to 15 kg


No. 20193-071

= 50

30193-080



Erbe MONOPlate 40, single, VIO, ICC, ACC, T-Series, contact surface 40 cm²



without connecting cable, for children < 5kg

No. 20193-073

= 50

30193-080



Connecting cables for return electrodes	Length	Piece	No.
Return electrode cable, VIO, ICC, ACC, T-Series, Standard, for return electrodes with contact stud	4 m 5 m	1 1	20194-077 20194-078
Return electrode cable, VIO, ICC, ACC, non-Erbe units, International, for return electrodes with split contact surface and contact stud	4 m 5 m	1 1	20194-080 20194-087
Return electrode cable, VIO, ICC, ACC, non-Erbe units, International, for return electrodes with single contact surface and contact stud	4 m 5 m	1 1	20194-079 20194-086

Return electrodes

Single use with connecting cable

Erbe NESSY Ω , split, VIO, non-Erbe units, International



contact surface 85 cm², equiptential ring 23 cm²,
with connecting cable 4 m


No. 20193-083

= 50

30193-082



Erbe NESSY Plate 170, split, VIO, ICC, ACC, non-Erbe units, International



contact surface 168 cm², with connecting cable 3 m


No. 20193-074

= 50

30193-080



Erbe NESSY Plate 70, split, VIO, ICC, ACC, non-Erbe units, International



contact surface 72 cm², with connecting cable 3 m,
for children from 5 to 15 kg

No. 20193-075

= 50


30193-080



Return electrodes

Reusable with contact stud

NESSY® RePlate 200, contact surface 194 cm², reusable, can be monitored

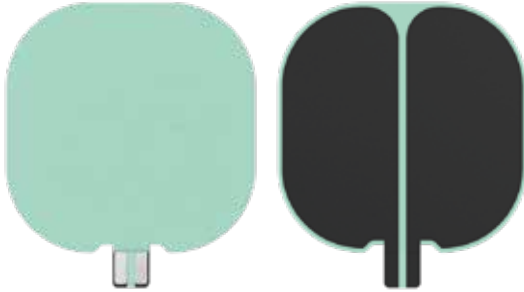

No. 20193-090

= 1

max 95 °C

30193-088

NESSY® RePlate Fixation, length 82 cm



No. 20193-091

= 1

max 95 °C

30193-088

Contact spray/Signaspray®, for NESSY® RePlate



No. 20193-092

= 1

D181820

Connecting cables for return electrodes	Length	Piece	No.
Return electrode cable, VIO, ICC, ACC, T-Series, Standard, for return electrodes with contact stud	4 m	1	20194-077 20194-078
	5 m	1	
Return electrode cable, VIO, ICC, ACC, non-Erbe units, International, for return electrodes with split contact surface and contact stud	4 m	1	20194-080 20194-087
	5 m	1	



Return electrodes

Reusable with contact stud

NESSY® RePlate kit I, reusable, incl. fixation and contact spray



No. 20193-093

= 1

max 95 °C

30193-088

NESSY® RePlate kit II, reusable, incl. fixation



No. 20193-094

= 1

max 95 °C

30193-088

Important information

The information, recommendations and other details contained in this medium ("information") reflect our state of knowledge and the state of the art in science and technology at the time the medium was created. The information is of a general nature, non-binding and intended solely for general information purposes; it does not constitute instructions for use.

The information and recommendations contained in this medium do not create any legal obligations on the part of Erbe Elektromedizin GmbH and its affiliated companies ("Erbe") or any other claims against Erbe. The information does not constitute any guarantees or other information on the nature of the product; such information requires an express contractual agreement with Erbe in each individual case.

Erbe is not liable for any kind of damage resulting from following the information on this medium, regardless of any legal grounds for liability.

Every user of an Erbe product is responsible for testing the respective Erbe product in advance with regard to its properties and its suitability for the intended type of use or purpose. Suitable type of use of the respective Erbe product can be found in the instructions for use for the respective Erbe product. The user is obliged to ascertain whether the instructions for use available to him/her correspond to the current status of the specific Erbe product. Devices may only be used in accordance with the instructions for use.

Information on settings, application sites, application duration and use of the respective Erbe product is based on the clinical experience of individual centers, physicians and clinical literature independent of Erbe as well as post market surveillance and empirical evidence. They constitute reference values, or Experienced Starting Settings, which must be checked by the user to ensure that they are suitable for the specifically planned application. Depending on the circumstances of a specific application, it may be necessary to deviate from the information provided. The user is responsible for checking this when using Erbe products. We wish to note that science and technology are subject to constant development as a result of research and clinical experience. Similarly, medicine and clinical application are constantly evolving as a result of research and technological development. This may also make it necessary for the user to deviate from the information provided on this medium.

This medium contains information about Erbe products that may not be approved/cleared in certain countries. The user of the respective Erbe product is obliged to inform himself/herself as to whether the Erbe product he/she is using is legally approved/cleared in his/her country and/or to what extent, if any, there are legal requirements for or restrictions on its use.

This medium is not intended for use in the USA.

Erbe Elektromedizin GmbH
Waldhoernlestrasse 17
72072 Tuebingen
Germany

Phone +49 7071 755-0
info@erbe-med.com
erbe-med.com
medical-videos.com